



# Novel automated processing techniques of fluorescein angiography (FA) images in patients with Uveitis

Natasha Kesav<sup>1</sup>, Qixin Yang<sup>2</sup>, Wolfgang Losert<sup>2</sup>, Jongwoo Kim<sup>3</sup>, Stefan Jaeger<sup>3</sup>, H. Nida Sen<sup>1</sup>

National Eye Institute  
Medical Research Scholars Program

<sup>1</sup>Laboratory of Immunology, National Eye Institute (NEI), Bethesda, MD, <sup>2</sup>Department of Physics, University of Maryland, College Park, MD, <sup>3</sup>Lister Hill National Center of Biomedical Communications, U.S. National Library of Medicine




A0135

## ABSTRACT


- Fluorescein angiography (FA) is a diagnostic imaging modality to visualize abnormalities in retinal and choroidal circulation such as vascular leakage.
- There is a need of objective quantification and detection of vascular pathology in uveitis.
- We demonstrate the potential of two novel automated processing techniques to detect leakage in FA images.**

## METHODS

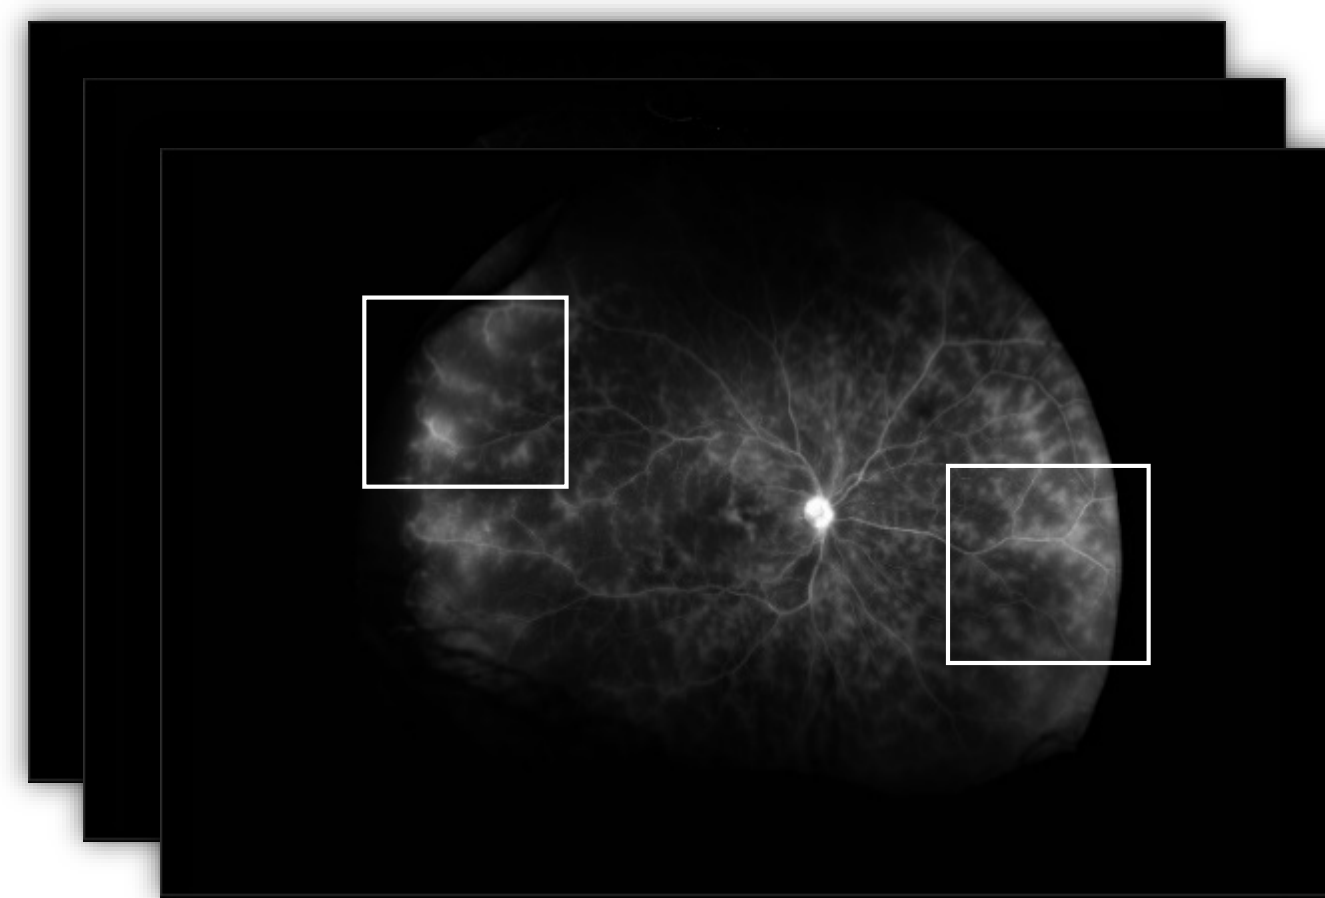


- Images used in this study belonged to patients enrolled in the Uveitis/Intraocular Inflammatory Biobank (iBank) protocol at the NEI who underwent FA using the Optos 200Tx (Optos plc, Dunfermline, United Kingdom)
- Individual early and mid-phase angiographic images were selected if vascular leakage was identified by expert readers.
- Patient images were excluded in the cases of poor image quality, media opacity and severe artifacts obscuring view.
- Angiographic Images were retrospectively downloaded, removed of patient identifying information, and exported to analysis software.


## APPROACH 1

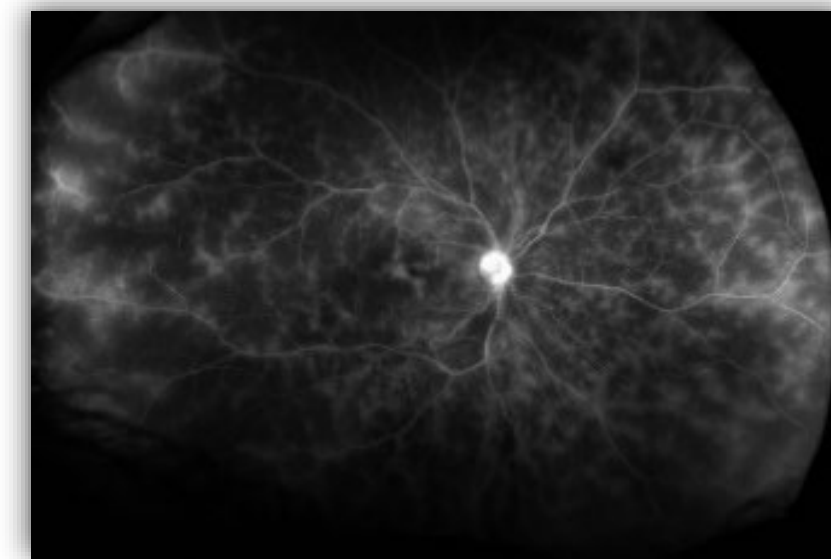


1. Pre-processing

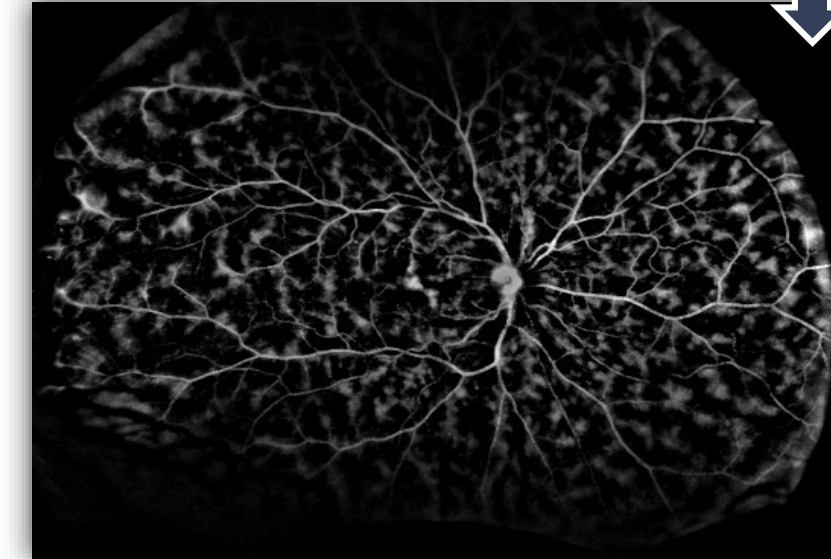


2. Adaptive binarization

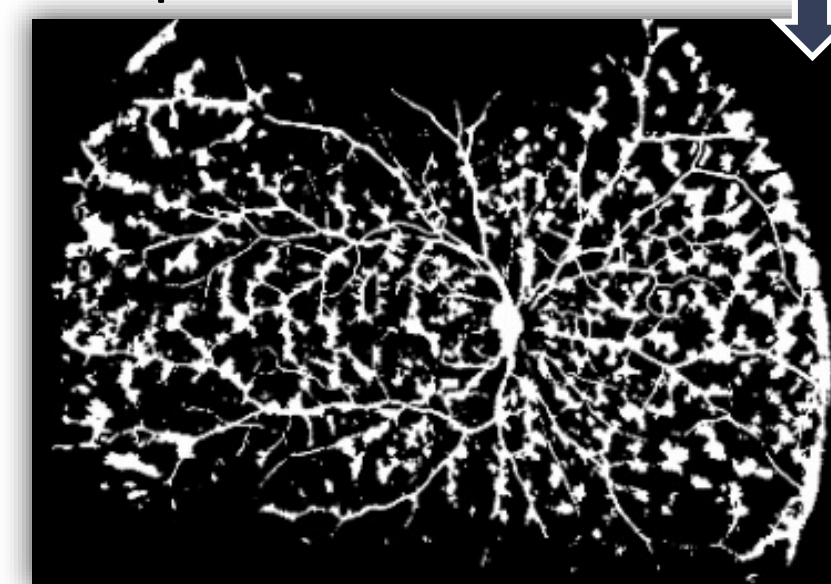

3. Detection of vasculature

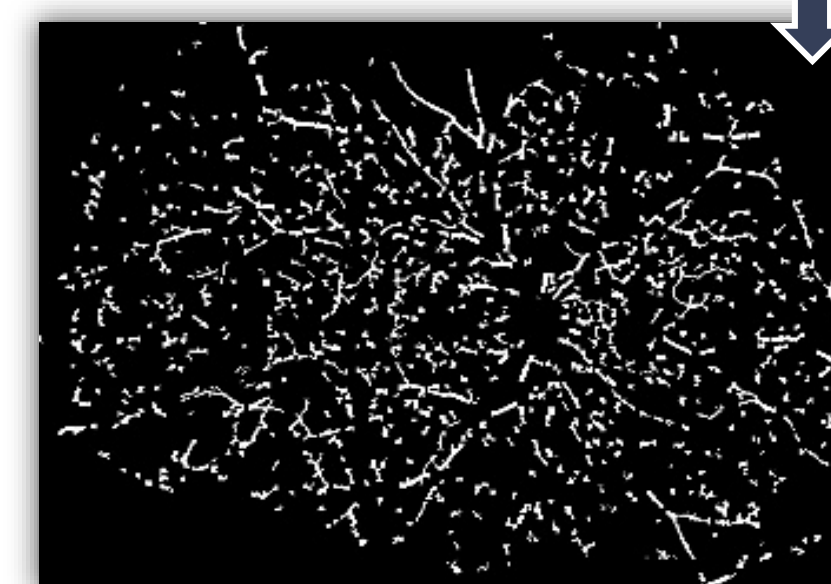


4. Vascular tree subtraction

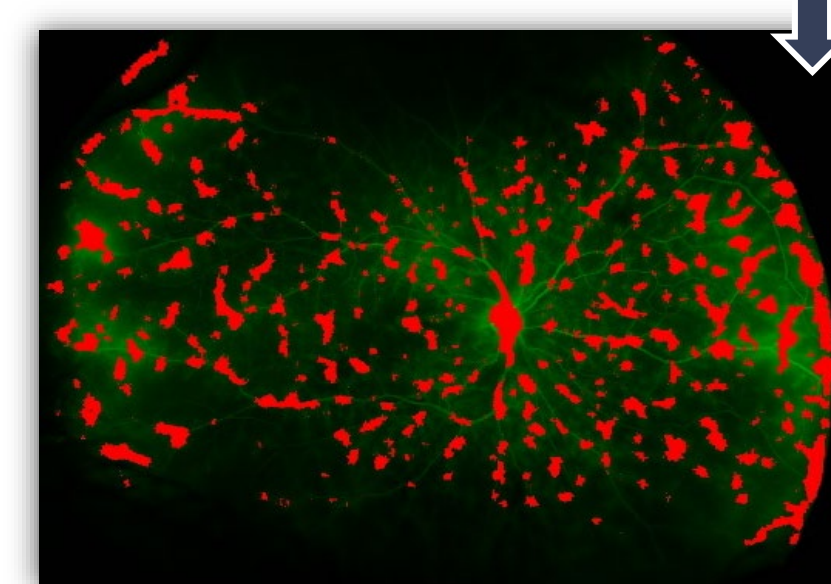


## APPROACH 2

1. Rotating Laplacian of Gaussian convolution in various angles

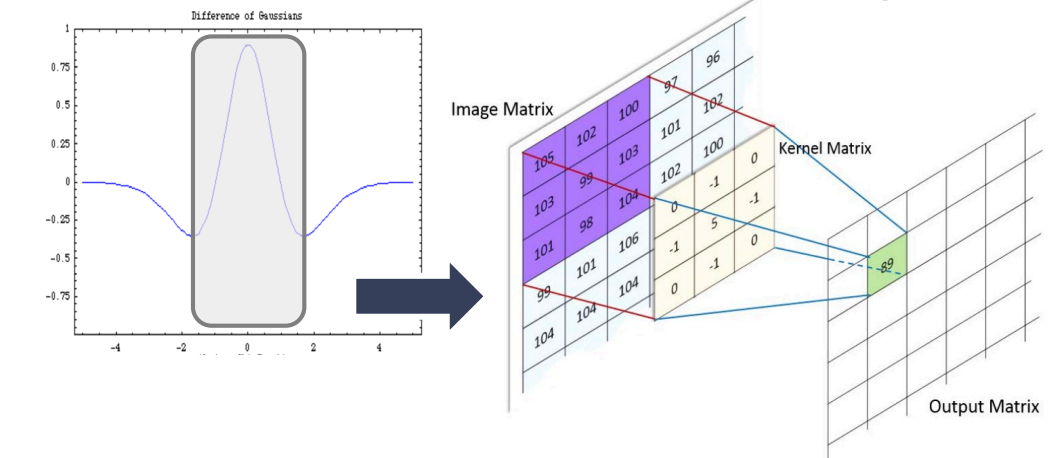


2. Convolve filters to max project onto one image and binarize

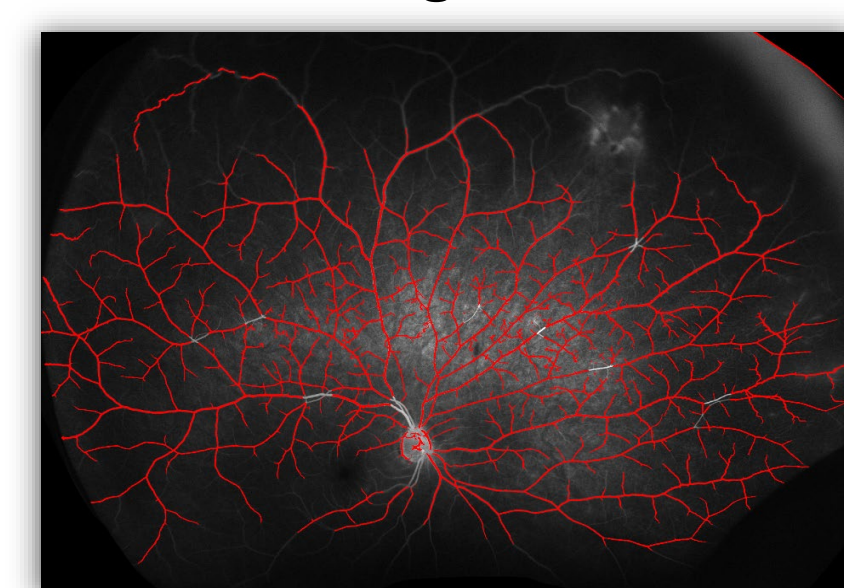


3. Detection of leakage using local pixel intensities + segmentation with Kmeans clustering



Further applications: Curvature calculation and junction detection

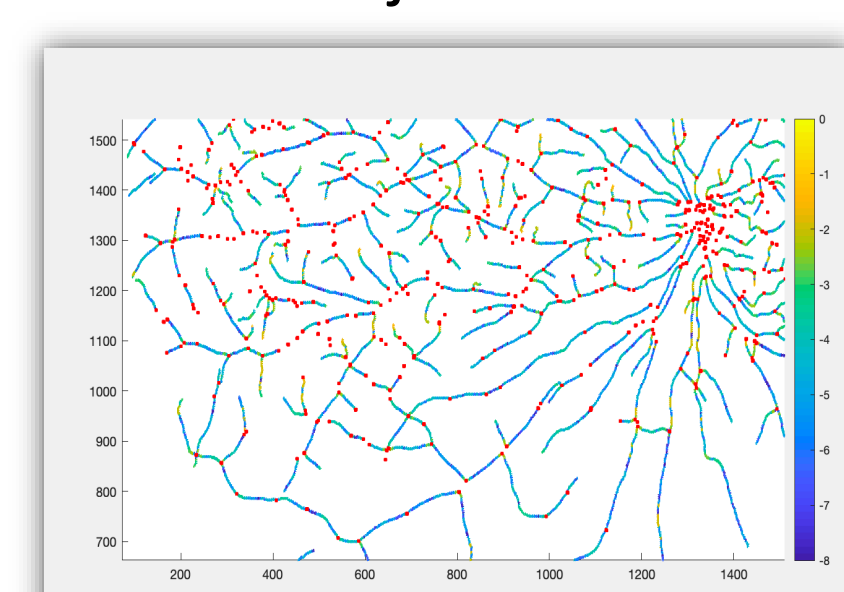

## RESULTS

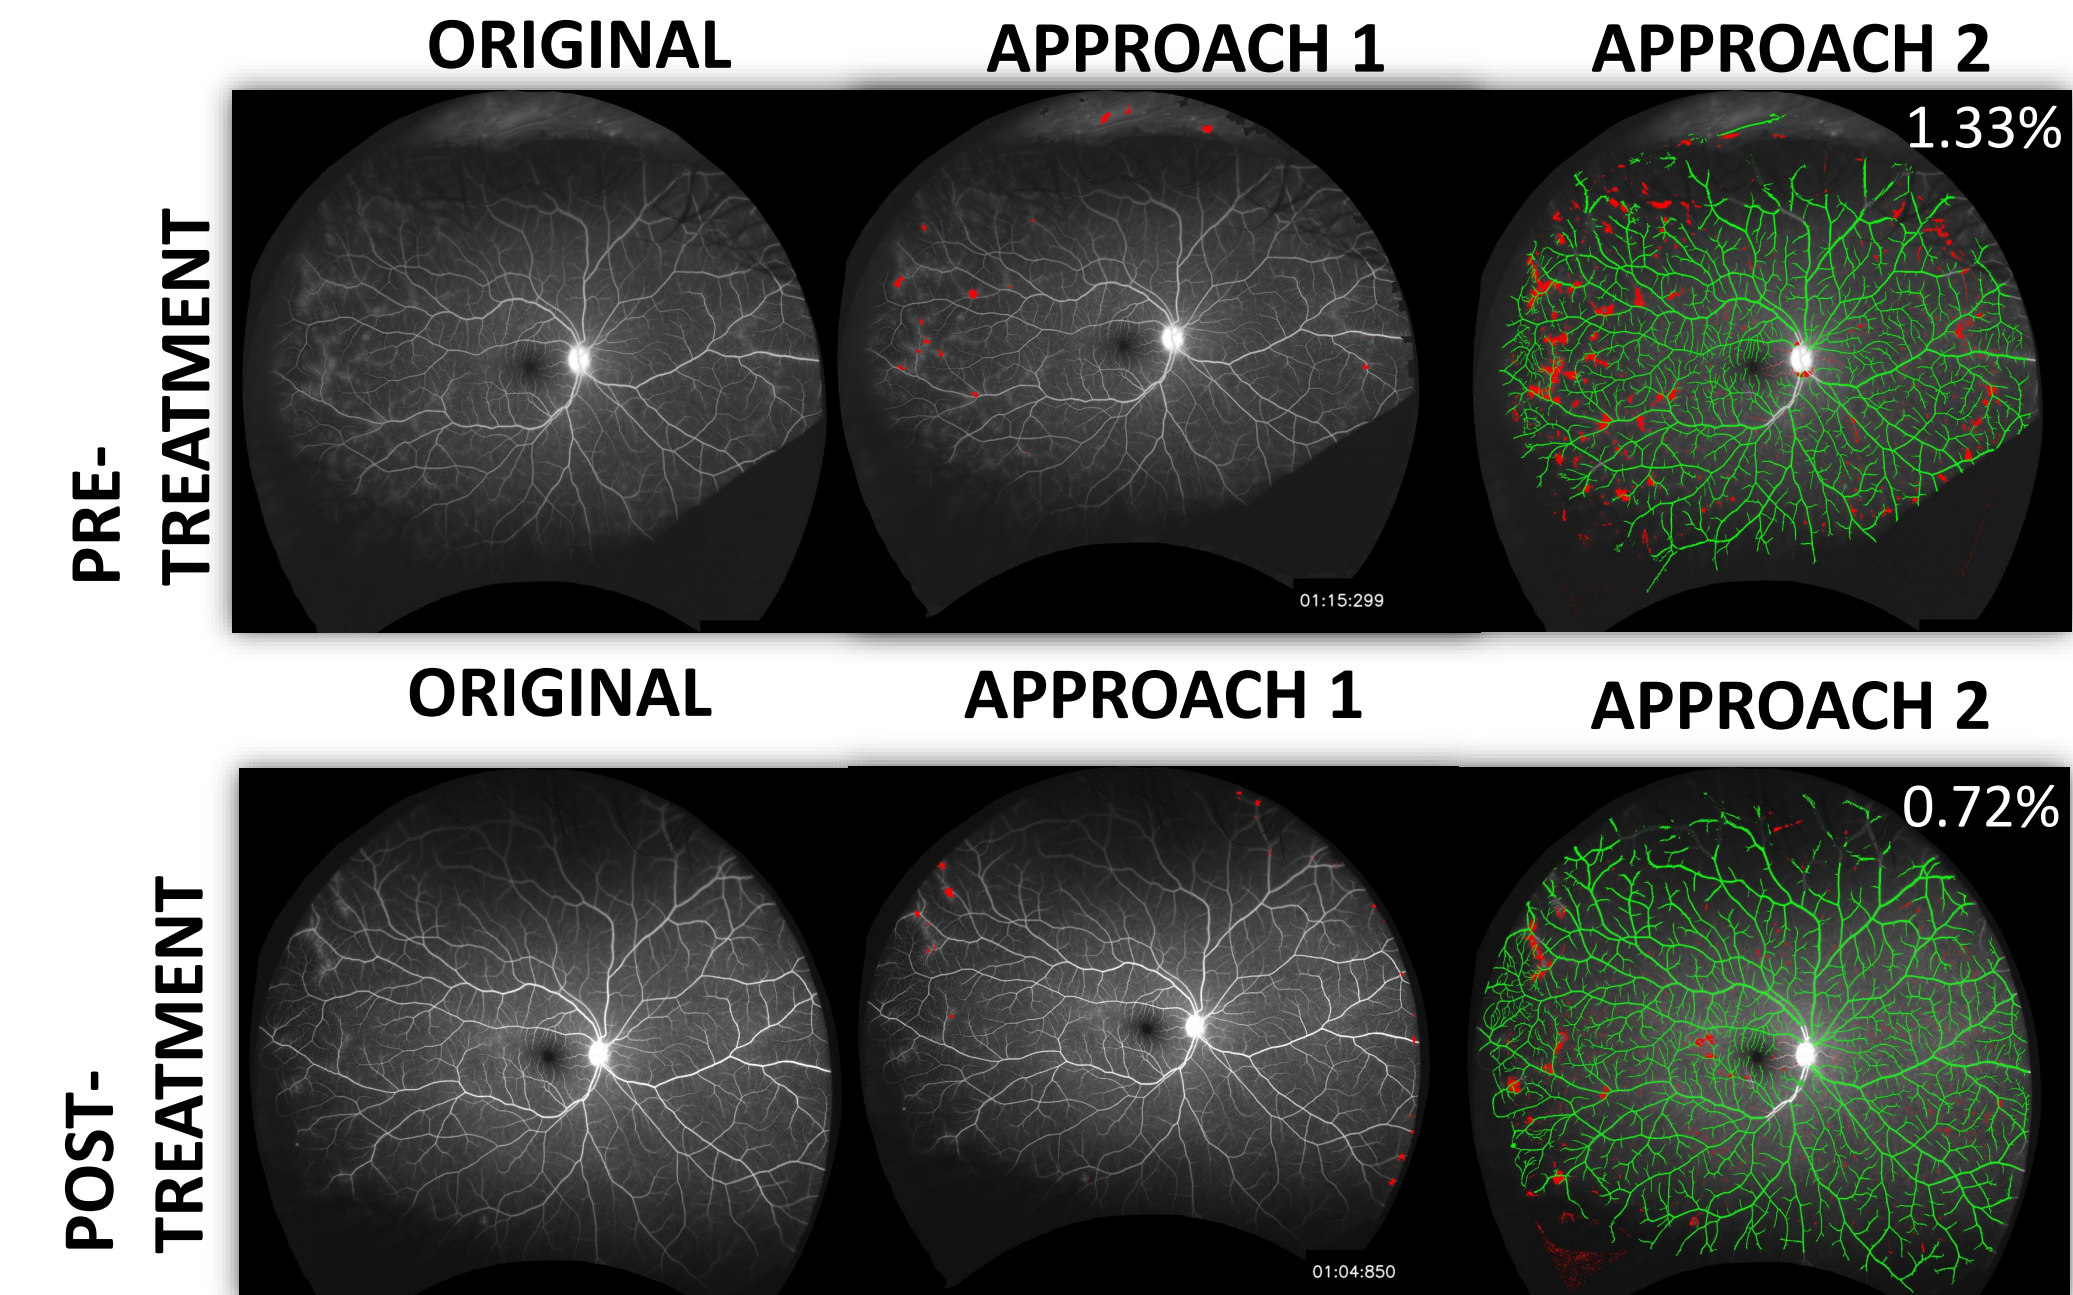

Application of **approach 1 and approach 2** before and after oral corticosteroids in a patient with mild vasculature leakage. Approach 2 demonstrates quantifiable improvement in leakage after treatment.

## LIMITATIONS & FUTURE DIRECTION

### Limitations:

- Different FOVs in FA videos in the same clinical practice
- Distortion of images due to eye movement and blinking
- Interframe motion cannot be modeled as rigid
- Uveitis: vitreous haze could confound visible media

### Future Directions:

- Refinement of algorithms + deep learning integration
- Reproducibility and repeatability across multicenter trials
- Explore skeleton structure as predictor/marker of disease

## CONCLUSION

**Our methods of FA image processing provides two novel algorithmic approaches to identifying leakage in patients with uveitis. Further refinement is warranted to apply to real-world patient care.**